



# CONCENTRICITY GAGES


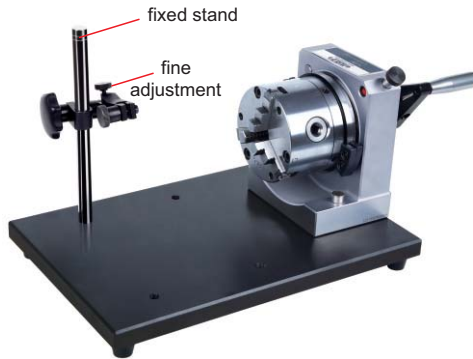


4786-1

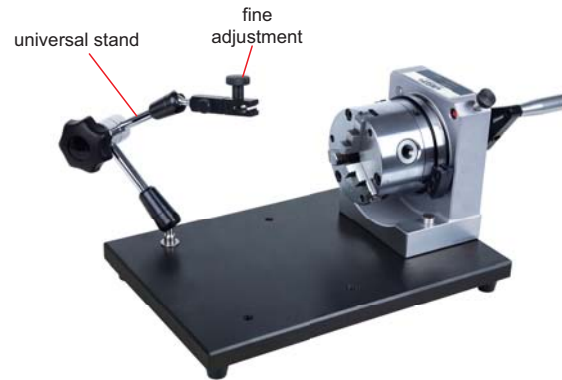

4786-2


to ensure the accuracy  $3\mu\text{m}$ , the distance between measuring point and roller should be  $<50\text{mm}$

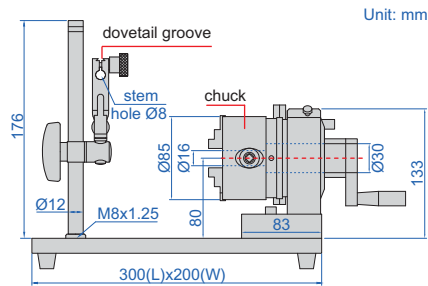

for cylinder



for tube



- Accuracy:  $3\mu\text{m}$
- $\varnothing 50\text{mm}$  setting ring and  $\varnothing 55\text{mm}$  calibration cylinder are included
- Optional accessory: dial test indicator

| Code   | Applicable inside diameter          | Applicable outside diameter        | Remark  |
|--------|-------------------------------------|------------------------------------|---|
| 4786-1 | $\varnothing 24\text{-}64\text{mm}$ | $\varnothing 2\text{-}70\text{mm}$ | fixed stand, high accuracy, inconvenient operation  |
| 4786-2 | $\varnothing 24\text{-}64\text{mm}$ | $\varnothing 2\text{-}70\text{mm}$ | universal stand, low accuracy, convenient operation |